



Proudly Owned and Operated in the USA

Searchable via: [FreedomDiagnosticsTesting.com](https://freedomdiagnostics.com)

Product	Bacteriostatic Water 10ml
Net Content	Replicate 1: 0.922% Replicate 2: 0.902%
Average Net Content	0.91 %

Certificate of Analysis

Accession Number	2604070091
Client	Peptide King
Search Code	Prot2604070091




Received Date:	04/07/2026
Reported Date:	04/9/2026

Lot	PH-BAC10-2026046
Purity	Replicate 1: 99.69% Replicate 2: 99.72%
Appearance	Clear Liquid

Endotoxin Threshold	Result
Replicate 1	Pass
Replicate 2	Pass

All Chemical Analysis was performed by HPLC with UV Detection Coupled with Mass Spectrometry

Mass Identification	Average Purity
Benzyl Alcohol	99.71%

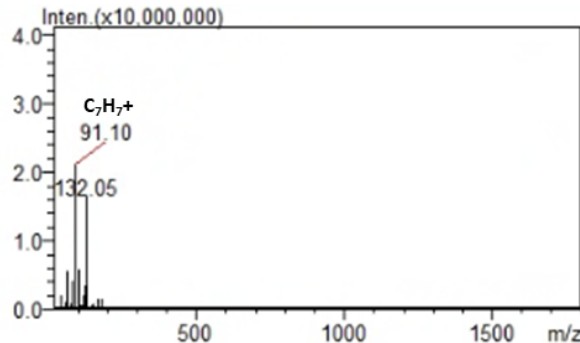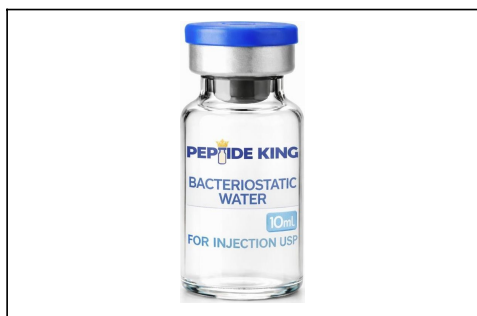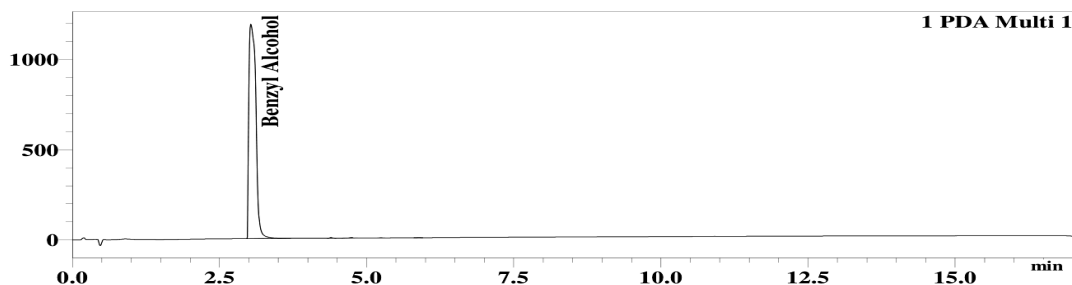

Alex Johnson

Alex Johnson
Principal Chemist

COA: 2604070091

The peptide purity analysis reported here was conducted using LCMS/MS under standard laboratory conditions. This analysis is intended for informational purposes only and is specific to the sample(s) provided. The peptides tested are intended for research use only and are not approved for human or veterinary use, diagnostic, therapeutic, or clinical applications. Results should be interpreted by qualified professionals within the scope of the intended research. The accuracy and reliability of the test may be influenced by sample integrity, handling, and other experimental variables.

Searchable via: [FreedomDiagnosticsTesting.com](https://freedomdiagnostics.com)

Contact at: Admin@FreedomDiagnostics.net